



**Starna scientific**  
'Setting the Standard'

## Quality Assurance in the Analytical Laboratory

# Spectrophotometer Visible Wavelength Qualification Didymium Glass Filters

### Purpose

Like its liquid counterpart, the didymium glass filter produces characteristic peaks that make it suitable for use as a wavelength reference material in the visible region of the spectrum.

### Description and Discussion

Glass filters mounted 'stress free' in an anodised aluminium holder. Glass filter containing didymium (a mixture of neodymium & praseodymium) oxide, mounted stress free in an anodised aluminium holder. As a solid material the didymium glass filter is physically more robust than the equivalent liquid cell, and can therefore be used in more demanding environments, making it especially useful as a routine wavelength check. Sliding window covers are provided to protect the surface from damage when not in use. Variations from melt to melt of the glass can cause small uncertainties in peak position, so each Starna filter is individually certified.


The spectrum shows 11 characteristic and well-defined peaks covering the wavelength range from 430 nm to 890 nm.



Approximate peak wavelength values (in nm) are:

431, 473, 513, 529, 573, 585, 685, 741, 749, 807, 879.

Note: The above values are for guidance only. Because the absorption bands are asymmetric, measured values will be spectral bandwidth dependent. The Calibration Certificate accompanying each Starna Didymium Glass Reference gives actual values measured at bandwidths of 0.10, 0.25, 0.50, 1.00, 1.50, 2.00 and 3.00 nm, and only these certified values should be used for instrument qualification. On request, Starna can provide certified values at other wavelengths and bandwidth values.

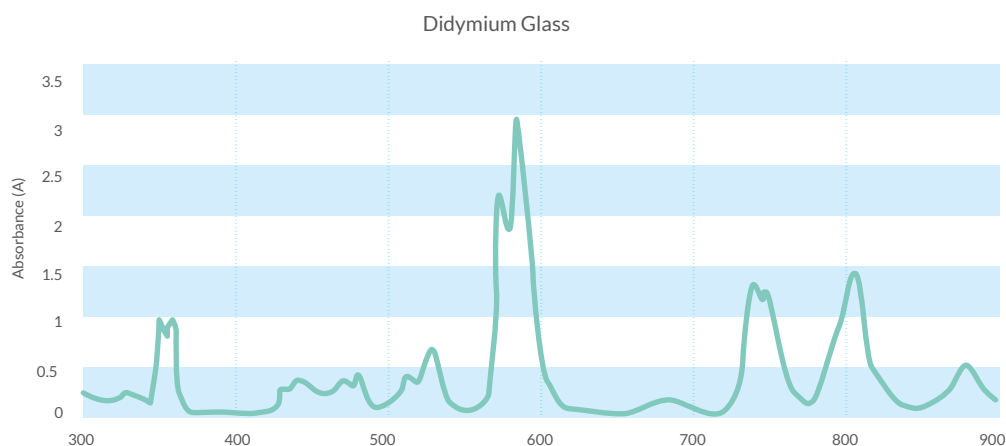

# Spectrophotometer Visible Wavelength Qualification

## Didymium Glass Filters

### Certification and Documentation

A Certificate of Calibration and Traceability and full instructions for use are provided with each Reference Material. The certificate is supplied in electronic format, on a USB drive in the same box as the references, allowing hard copy to be produced on demand and giving easy interface to the user's own IT systems. Certification measurements are made on a reference spectrophotometer that has been qualified using Standard Reference Materials certified by the National Institute of Standards and Technology (NIST) in the USA, or against primary physical references such as elemental emission lines.

### Warranty

STARNA offers a Lifetime Guarantee on all Starna Certified Reference Materials, unless otherwise stated, such that any reference material that moves outside its published uncertainty budget will be replaced free of charge. This guarantee is subject to the reference materials being re-certified at least every two years and that the references have not been physically, thermally or optically abused. The STARNA UKAS accredited calibration laboratory aims to re-certify and despatch references within five working days from receipt.

### Accreditation

Starna Scientific is accredited to both ISO 17034 as a Reference Material producer, and ISO/IEC 17025 as a Calibration Laboratory for optical reference measurements. Starna Scientific's manufacturing facility is accredited to the ISO 9001 Quality Management System with BSI. For details see [www.starna.com/accreditations](http://www.starna.com/accreditations).

### How to Order

| CATALOGUE<br>NUMBER   |       |
|-----------------------|-------|
| Didymium glass filter | RM-DG |



**Starna** scientific  
'Setting the Standard'

[www.starna.com](http://www.starna.com)  
[sales@starna.com](mailto:sales@starna.com)  
+ 44 (0) 20 8501 5550